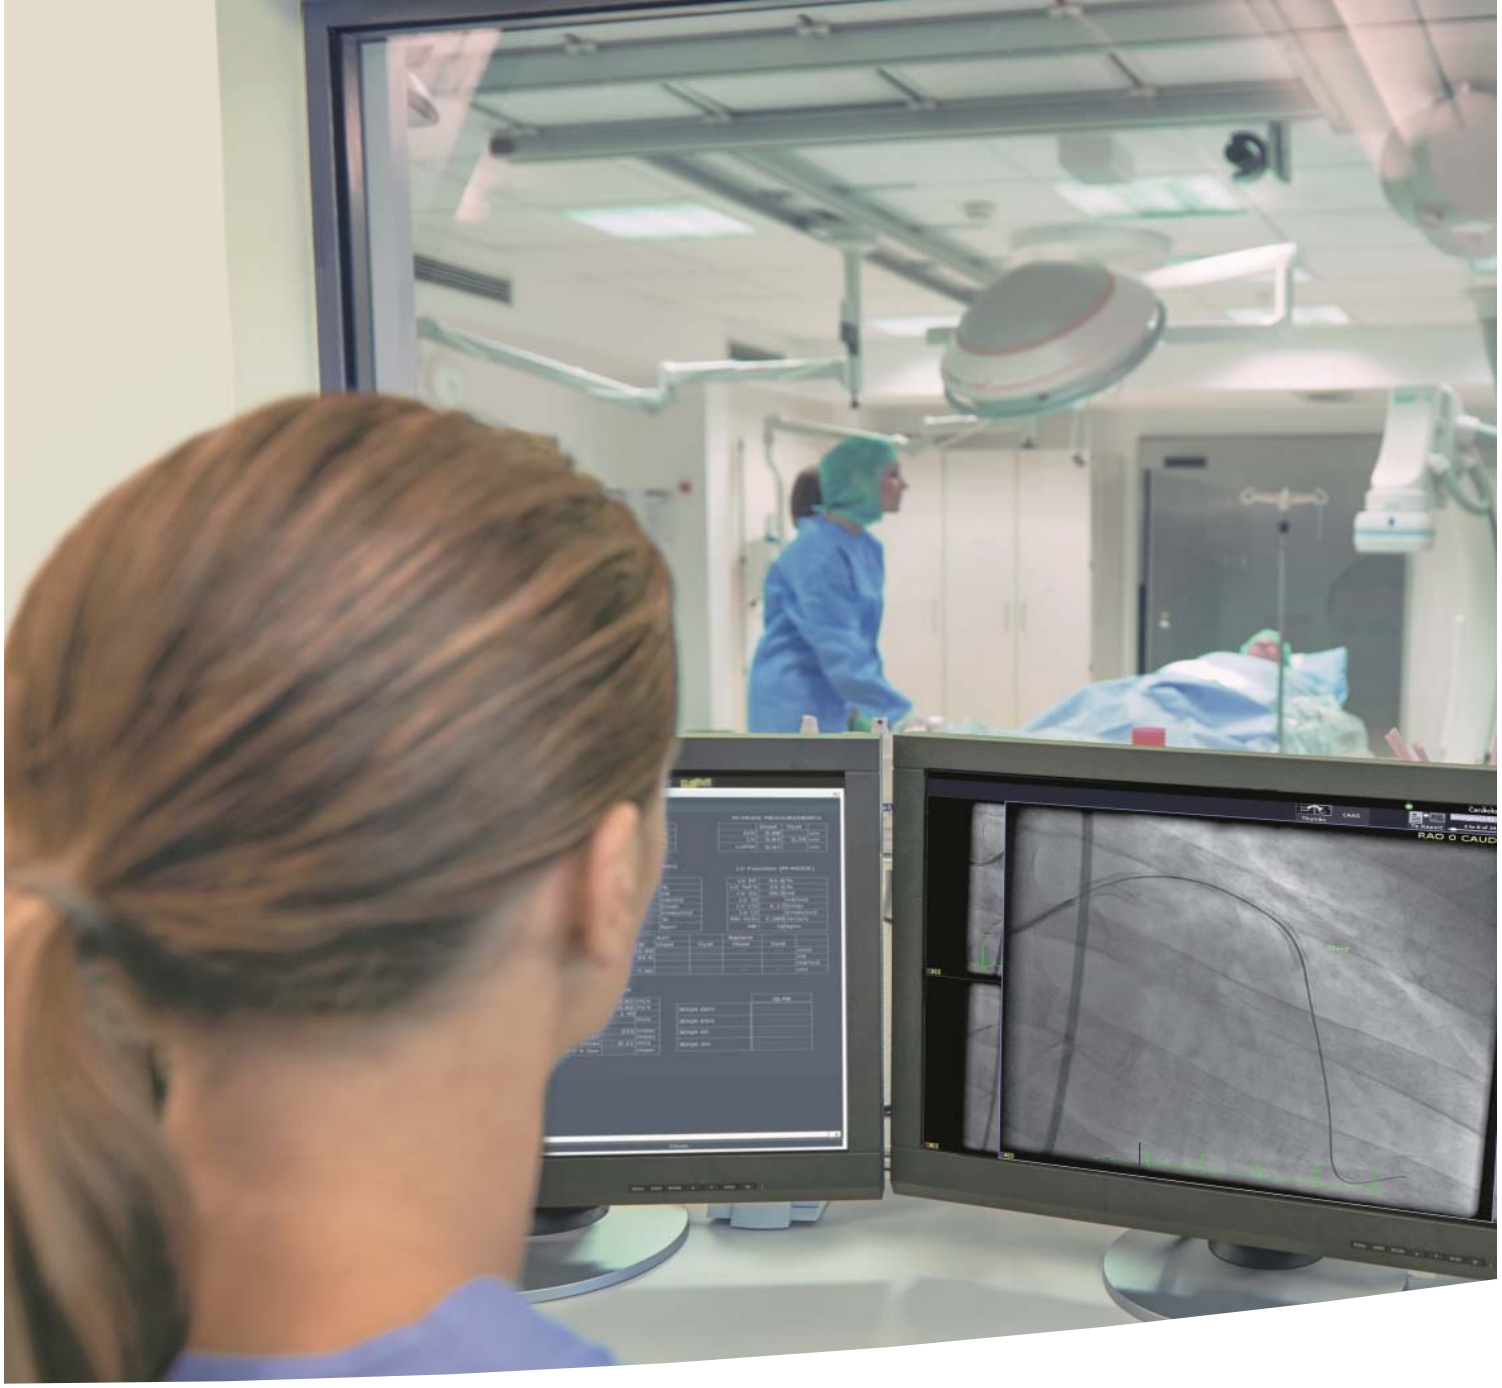

DICOM Conformance Statement

syngo® Dynamics

Dicom Image Review

VA30

Last Updated: January-14, 2019

siemens.com/healthineers

SIEMENS Healthineers

Table of Contents

1 Introduction 3
1.1 Purpose of this Document 3
1.1.1 Image Display Support (Software) 3
1.2 Limitations 5
1.3 Sources for this Document 5
1.4 Acronyms and Abbreviations 5
2 Network Conformance Statement 6
2.1 Introduction 6
2.2 Implementation Model 6
2.2.1 Sequencing of Real World Activities 6
2.3 Communication Profiles 6
2.3.1 Supported Communications Stacks 6
2.3.2 OSI Stack 6
2.3.3 Point-to-Point Stack 6

List of Tables

Table 1.1-1 Software Review Supported Image Formats 5

© Siemens Healthcare GmbH / Siemens Medical Solutions USA, Inc., 2019. All rights reserved.

1 Introduction

1.1 Purpose of this Document

This document is a DICOM Conformance Statement for the DICOM Image Review (DIR).

The DIR provides diagnostic display of DICOM Images conforming to the Ultrasound Image Storage, Ultrasound Multi-frame Image Storage, X-ray Angiographic Image Storage and Secondary Capture Image Storage SOP Classes. Images are reviewed through the DICOM Image Review component which displays DICOM images without any additional compression. The DIR is part of the Siemens *syngo*® Suite and is designed to operate in conjunction with the *syngo*® Dynamics Server. The DIR uses DICOM as an external interface standard. Non-DICOM internal communication mechanisms between the DIR and the *syngo*® Dynamics Server are used for the transfer and display of images.

The DIR provides support for the DICOM US Region Calibration Module. When ultrasound images contain this module, the DIR is able to interpret the region calibration data provided by the ultrasound acquisition unit. Standard pixel spacing attributes are also supported if provided with ultrasound captures. The DIR provides support for the DICOM Imager Pixel Spacing and Estimated Radiographic Magnification Factor attributes often sent with X-Ray Angiographic captures. When XA captures contain this data the DIR can interpret them. In the case where no calibration data is provided by the acquisition device, captures may be manually calibrated using the DIR.

1.1.1 Image Display Support (Software)

The DIR displays Ultrasound and X-Ray Angiographic images from the *syngo*® Dynamics Server.

The DIR supports the image formats shown in Table 1.1-1 when displaying images using software. The DIR supports the display of 8, 10, 12 and 16 bit image formats.

© Siemens Healthcare GmbH / Siemens Medical Solutions USA, Inc., 2019. All rights reserved.

Photometric Interpretation	Transfer Syntax	Planar Configuration
MONOCHROME1	Uncompressed Implicit VR Little Endian 1.2.840.10008.1.2	N/A
	Uncompressed Explicit VR Little Endian 1.2.840.10008.1.2.1	N/A
	RLE Lossless Image Compression 1.2.840.10008.1.2.5	N/A
	JPEG Lossy Baseline (Process 1) 1.2.840.10008.1.2.4.50	N/A
	JPEG Lossless, Non-Hierarchical (Process 14) 1.2.840.10008.1.2.4.57	N/A
	JPEG Lossless, Non-Hierarchical (Process 14) 1.2.840.10008.1.2.4.70	N/A
MONOCHROME2	Uncompressed Implicit VR Little Endian 1.2.840.10008.1.2	N/A
	Uncompressed Explicit VR Little Endian 1.2.840.10008.1.2.1	N/A
	RLE Lossless Image Compression 1.2.840.10008.1.2.5	N/A
	JPEG Lossy Baseline (Process 1) 1.2.840.10008.1.2.4.50	N/A
	JPEG Lossless, Non-Hierarchical (Process 14) 1.2.840.10008.1.2.4.57	N/A
	JPEG Lossless, Non-Hierarchical (Process 14) 1.2.840.10008.1.2.4.70	N/A
RGB	Uncompressed Implicit VR Little Endian 1.2.840.10008.1.2	0 - Chunky
	Uncompressed Implicit VR Little Endian 1.2.840.10008.1.2	1 - Planar
	Uncompressed Explicit VR Little Endian 1.2.840.10008.1.2.1	0 - Chunky
	Uncompressed Explicit VR Little Endian 1.2.840.10008.1.2.1	1 - Planar
	JPEG Lossless, Non-Hierarchical (Process 14) 1.2.840.10008.1.2.4.70	0 - Chunky
	JPEG Lossless, Non-Hierarchical (Process 14) 1.2.840.10008.1.2.4.70	1 - Planar
YBR_FULL	Uncompressed Implicit VR Little Endian 1.2.840.10008.1.2	0 - Chunky
	Uncompressed Explicit VR Little Endian 1.2.840.10008.1.2.1	0 - Chunky
	RLE Lossless Image Compression 1.2.840.10008.1.2.5	0 - Chunky
	RLE Lossless Image Compression 1.2.840.10008.1.2.5	1 - Planar

© Siemens Healthcare GmbH / Siemens Medical Solutions USA, Inc., 2019. All rights reserved.

Photometric Interpretation	Transfer Syntax	Planar Configuration
MONOCHROME1	Uncompressed Implicit VR Little Endian 1.2.840.10008.1.2	N/A
	Uncompressed Explicit VR Little Endian 1.2.840.10008.1.2.1	N/A
	RLE Lossless Image Compression 1.2.840.10008.1.2.5	N/A
	JPEG Lossy Baseline (Process 1) 1.2.840.10008.1.2.4.50	N/A
	JPEG Lossless, Non-Hierarchical (Process 14) 1.2.840.10008.1.2.4.57	N/A
	JPEG Lossless, Non-Hierarchical (Process 14) 1.2.840.10008.1.2.4.70	N/A
	JPEG Lossless, Non-Hierarchical (Process 14) 1.2.840.10008.1.2.4.70	0 - Chunky
YBR_FULL_422	Uncompressed Implicit VR Little Endian 1.2.840.10008.1.2	0 - Chunky
	Uncompressed Explicit VR Little Endian 1.2.840.10008.1.2.1	0 - Chunky
	JPEG Lossy Baseline (Process 1) 1.2.840.10008.1.2.4.50	0

Table 1.1-1 Software Review Supported Image Formats

1.2 Limitations

None

1.3 Sources for this Document

ACR-NEMA Digital Imaging and Communications in Medicine (DICOM) Version 3 Parts 1 – 20.

1.4 Acronyms and Abbreviations

The following Acronyms and abbreviations are used in this document:

- ACR American College of Radiology
- AE Application Entity
- DICOM Digital Imaging and Communications in Medicine
- DIR DICOM Image Review
- NEMA National Electrical Manufacturers Association
- OQV Original Quality Viewer
- SCP Service Class Provider

© Siemens Healthcare GmbH / Siemens Medical Solutions USA, Inc., 2019. All rights reserved.

- SCU Service Class User
- SOP Service Object Pair
- SR Structured Report
- TCP/IP Transmission Control Protocol/Internet Protocol

2 Network Conformance Statement

2.1 Introduction

This section of the DICOM conformance statement specifies the compliance to the DICOM conformance requirements for the relevant Networking features of the *DIR*. Note that the format of this section follows the format described in DICOM Standard PS 3.2 (Conformance). Please refer to that part of the standard while reading this section.

The DIR is a medical imaging workstation designed to provide diagnostic review of Ultrasound images and X-Ray Angiographic images. It operates in conjunction with the *syngo*® Dynamics Server or compatible DICOM data provider for retrieval and display of images. Refer to the *syngo*® Dynamics Server DICOM Conformance Statement for a description of the *syngo*® Dynamics Server's DICOM capabilities.

2.2 Implementation Model

Not Applicable

2.2.1 Sequencing of Real World Activities

Not Applicable

2.3 Communication Profiles

2.3.1 Supported Communications Stacks

Not Supported

2.3.2 OSI Stack

Not Supported.

2.3.3 Point-to-Point Stack

Not Supported.

© Siemens Healthcare GmbH / Siemens Medical Solutions USA, Inc., 2019. All rights reserved.

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens Healthineers sales organization worldwide. Availability and packaging may vary by country and are subject to change without prior notice.

Some/All of the features and products described herein may not be available in the United States or other countries.

The information in this document contains general technical descriptions of specifications and options as well as standard and optional features that do not always have to be present in individual cases.

Siemens Healthineers reserves the right to modify the design, packaging, specifications and options described herein without prior notice. Please contact your local Siemens Healthineers sales representative for the most current information.

In the interest of complying with legal requirements concerning the environmental compatibility of our products (protection of natural resources and waste conservation), we recycle certain components. Using the same extensive quality assurance measures as for factory- new components, we guarantee the quality of these recycled components.

Note: Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Caution: Federal law restricts this device to sale by or on the order of a physician.

Siemens Healthineers Headquarters

Legal Manufacterer
Siemens Healthcare GmbH
Henkestr 127
91052 Erlangen
Germany

Telephone: +49 9131 84-0
siemens.com/healthineers

© Siemens Healthcare GmbH / Siemens Medical Solutions USA, Inc., 2019. All rights reserved.